Gima S.p.A. – Via Marconi, 1 - 20060 Gessate (MI) Italy
Italia: tel 199 400 401 – fax 199 400 403 – gima@gimaitaly.com
Export: phone + 39 02 953854209/221/225 – fax + 39 02 95380056

COD. 28180

USER MANUAL - HAND SUCTION UNIT

SYMBOLS:

Symbol	Definition of Symbol
	ATTENTION: See Instructions for Use
	Symbol for “KEEP AWAY FROM SUNLIGHT”
	Symbol for “KEEP DRY”
	CE mark has been identified according to Article 17 of the MDD (93/42/EEC)
	Symbol for “BATCH CODE”
	This symbol shall be accompanied by the name and the address of the manufacturer
	Symbol for “CATALOGUE NUMBER”

1. Product description

The suction device is a light portable suction unit that can be powered by one hand and allows the other hand free for other important duties. This suction unit was designed to provide simple operation and maintenance.

2. Product intended use

The suction device is intended to provide quick and effective pharyngeal and tracheal suction for multiple emergencies.

3. Specifications

Vacuum (max): -400mmHg
Peak free airflow: >20 l/min
Disposable container volume: 250ML
External diameter of catheter connection: 10mm and 6mm
Operating environmental temperature: -20 centigrade to + 50 centigrade (-4 F TO 122 F)
Storage environmental temperature: -40 centigrade + 60 centigrade (-4 F to 140F)
Dimension: 230*60*190mm

4. Operating Instruction

(1) Select appropriate size tubing (according to the size of the patient) and attach it to the adapter (if not attached already).

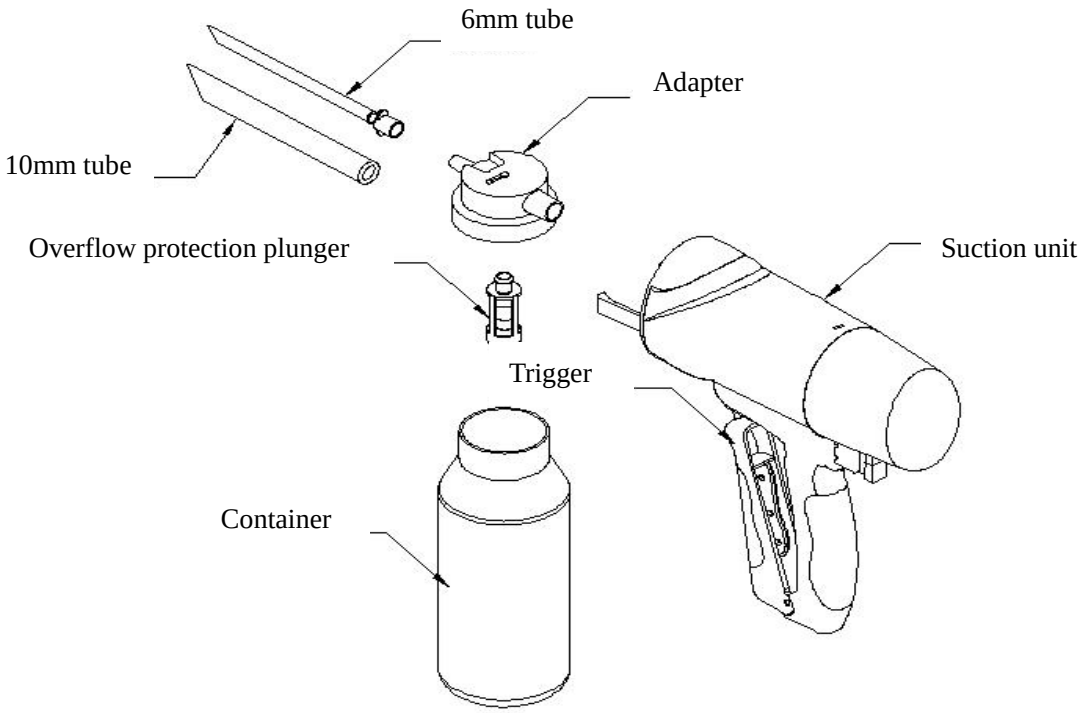

(2) Attach the adapter with tubing to the cap of the container. The container should be attached to the pump.

(3) The suction device is operated by a simple squeezing action of the trigger. Pull or squeeze the trigger toward the pump handle. This squeezing mechanism will generate the vacuum in the pump and suck the fluids into the container.

(4) There is an overflow protection plunger on the suction device. Once the protection device is operating, the fluid will not be absorbed into the suction device. And then the suction device will impossible to continue the operation of suction. At this moment, container should be substituted and then go along the operation.

(5) Once suction is completed, remove tubing slowly from the patient. Remove filled container by unsnapping the container (and tubing) from the pump. Place container along with the tubing in the poly bag. Discard disposable tubing and container appropriately.

(6) If required, place a label on the container for transportation to the laboratory.

5. Cleaning and Storage

Disinfect the pump and handle (by scrubbing with warm soapy water, mild detergent, bleach solution etc.) before placing into storage.

The pump requires no special maintenance or storage conditions.

6. Testing for correct function

Check the handle's condition and the pump function before returning it to service. Mount a container, occlude the suction port by thumb and pull or squeeze the pump handle to check for the vacuum.

This product includes a suction main body, adapter, container and each 10mm and 6mm sucker.

7. Caution

(1) It is important to read the manual carefully before operate.

(2) If the pump handle becomes difficult to operate, a blockage may have occurred. Do not continue suctioning until the source of the blockage has been determined (remove the blockage from the catheter, the adapter or the cap).

(3) If the pump is turned upside down, the overfill protection mechanism will be engaged making it impossible to suction.

GIMA WARRANTY CONDITIONS

Congratulations for purchasing a GIMA product. This product meets high qualitative standards both as regards the material and the production. The warranty is valid for 12 months from the date of supply of GIMA. During the period of validity of the warranty, GIMA will repair and/or replace free of charge all the defected parts due to production reasons. Labor costs and personnel traveling expenses and packaging not included. All components subject to wear are not included in the warranty. The repair or replacement performed during the warranty period shall not extend the warranty. The warranty is void in the following cases: repairs performed by unauthorized personnel or with non-original spare parts, defects caused by negligence or incorrect use. The warranty is void if the above regulations are not observed and if the serial code (if available) has been removed, cancelled or changed. The defected products must be returned only to the dealer the product was purchased from. Products sent to GIMA will be rejected.

David Medical Products (Su Zhou) Co., LTD.
88 FUDA,. LUDU, TAICANG SUZHOU, JIANGSU, 215412 CHINA